

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.

See for example, Seng and Dr. Z.
System of Sound
Therapy

each position
adjustable

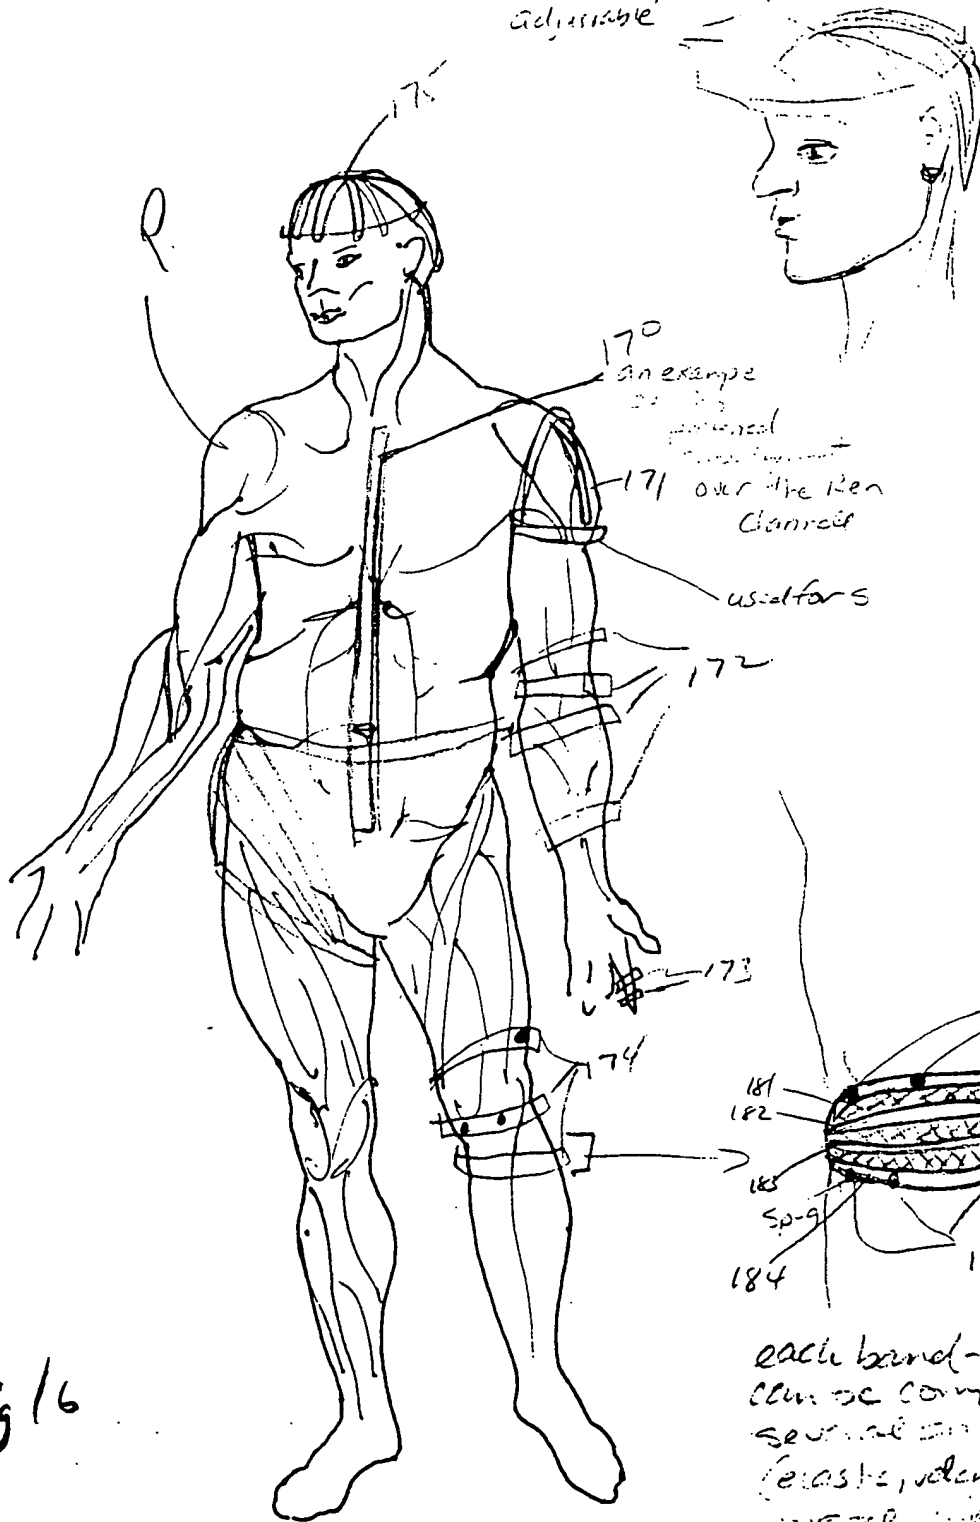


Fig 16

each band - all adjustable
element composed of
several smaller straps
(elastic, velcro, pliable shear
metal, with adjustable
position of magnets, polariz
packets, moxa and/or
medicaments utilizing the
techniques + principles of the previously described applicat.

10449393-112609

For
Hip
Knee,
Shoulder
injury or
Replacement
therapy

These straps can be
arranged in many
different configurations
and designs for each
individual's needs and
anatomy, and can be
used in conjunction
with other therapy devices
if desired.

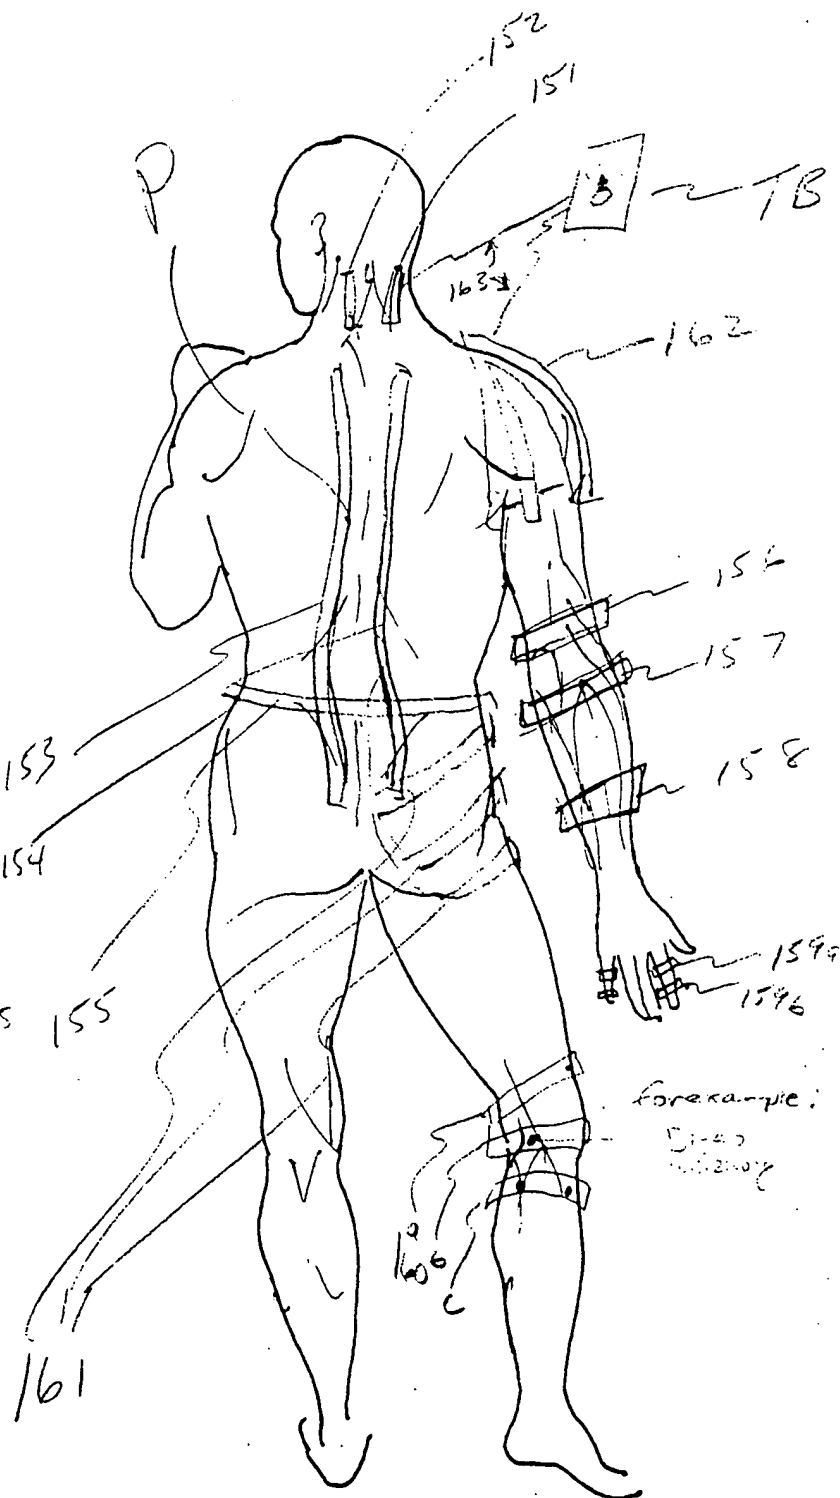
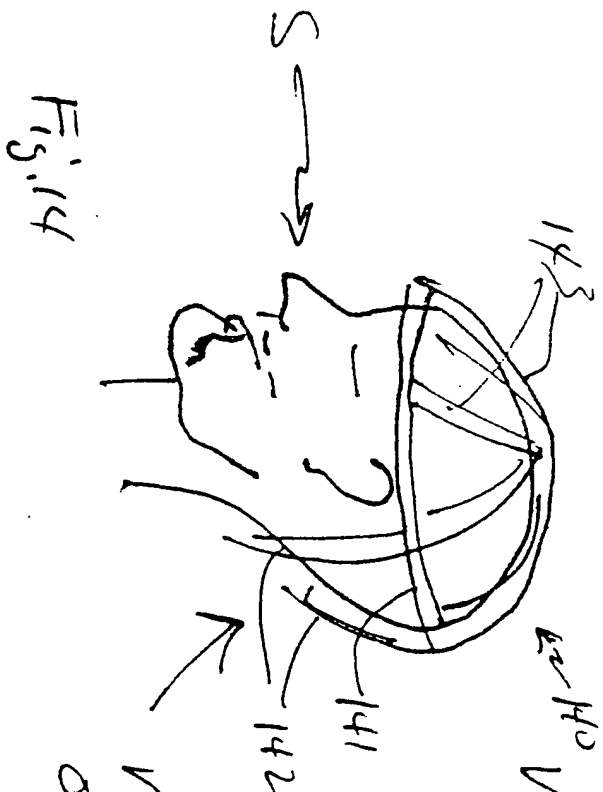




Fig. 15

+ totally adjustable
+ inexpensive to make

Remind you of something out of the Baker museum?

[illegible]

PRINT OF DRAWINGS
AS ORIGINALLY FILED

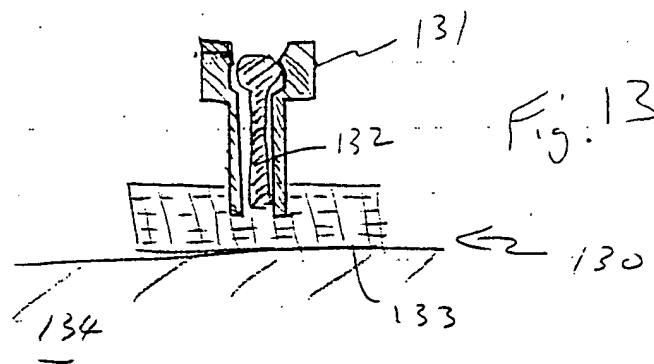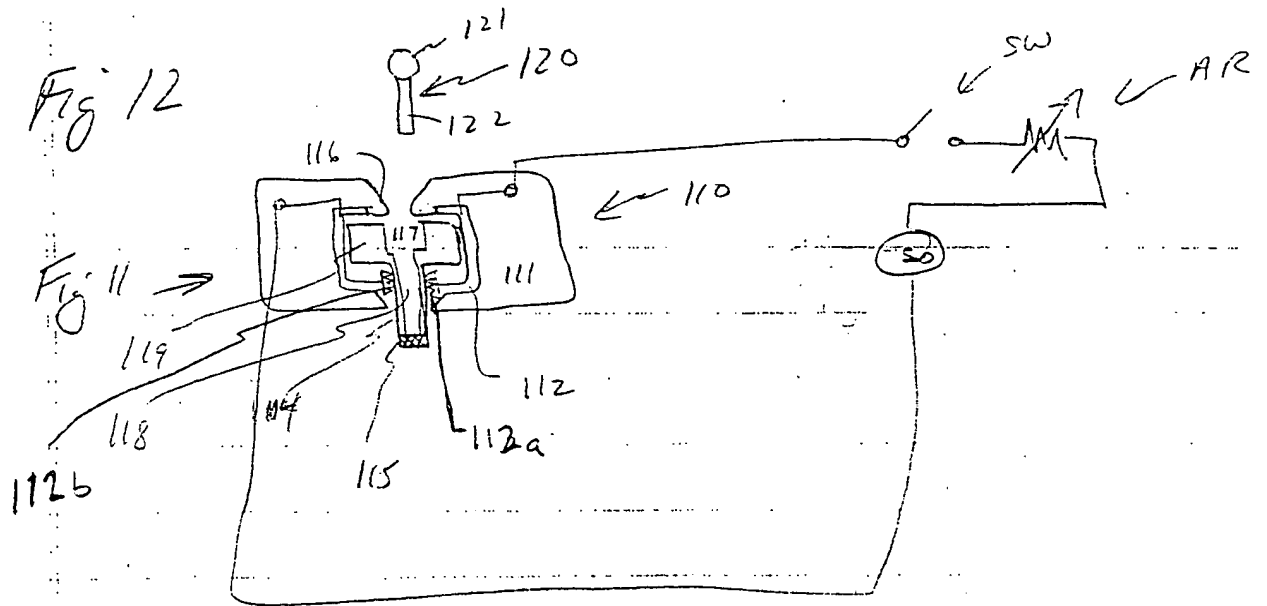

00449393-112509

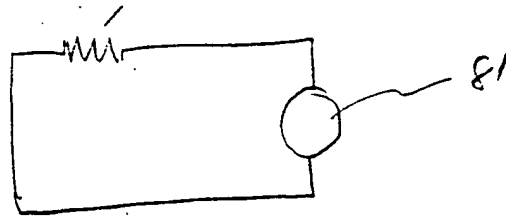


Fig. 7

80

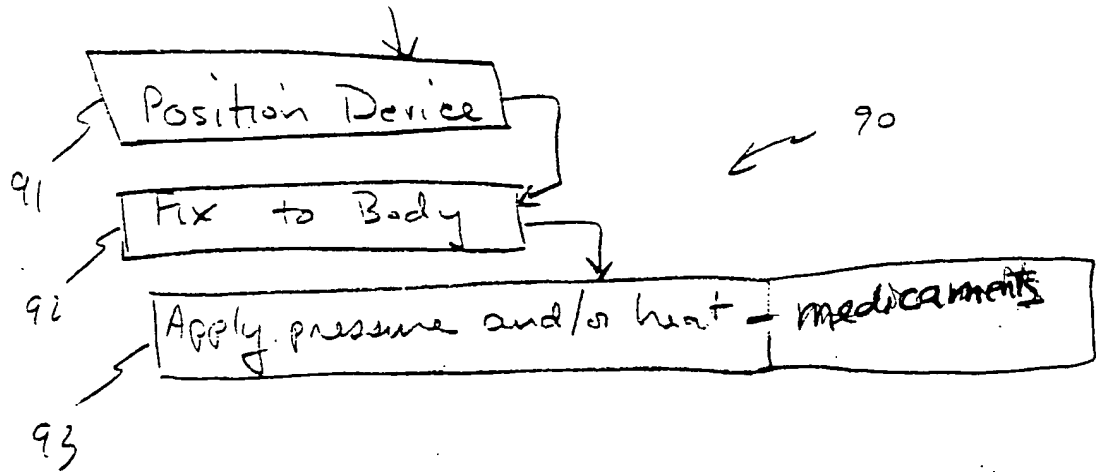


Fig. 8

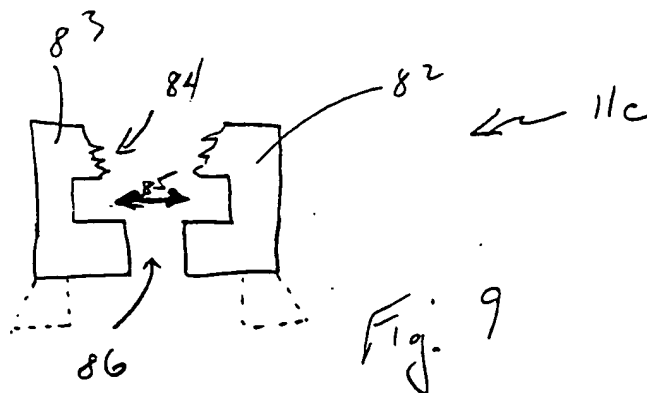


Fig. 9

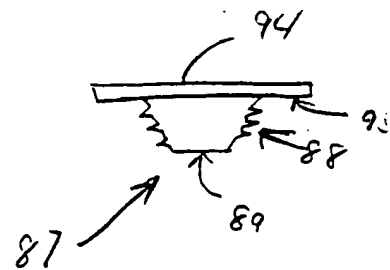


Fig. 10

00449393-112699

PRINT OF DRAWINGS
AS ORIGINALLY FILED

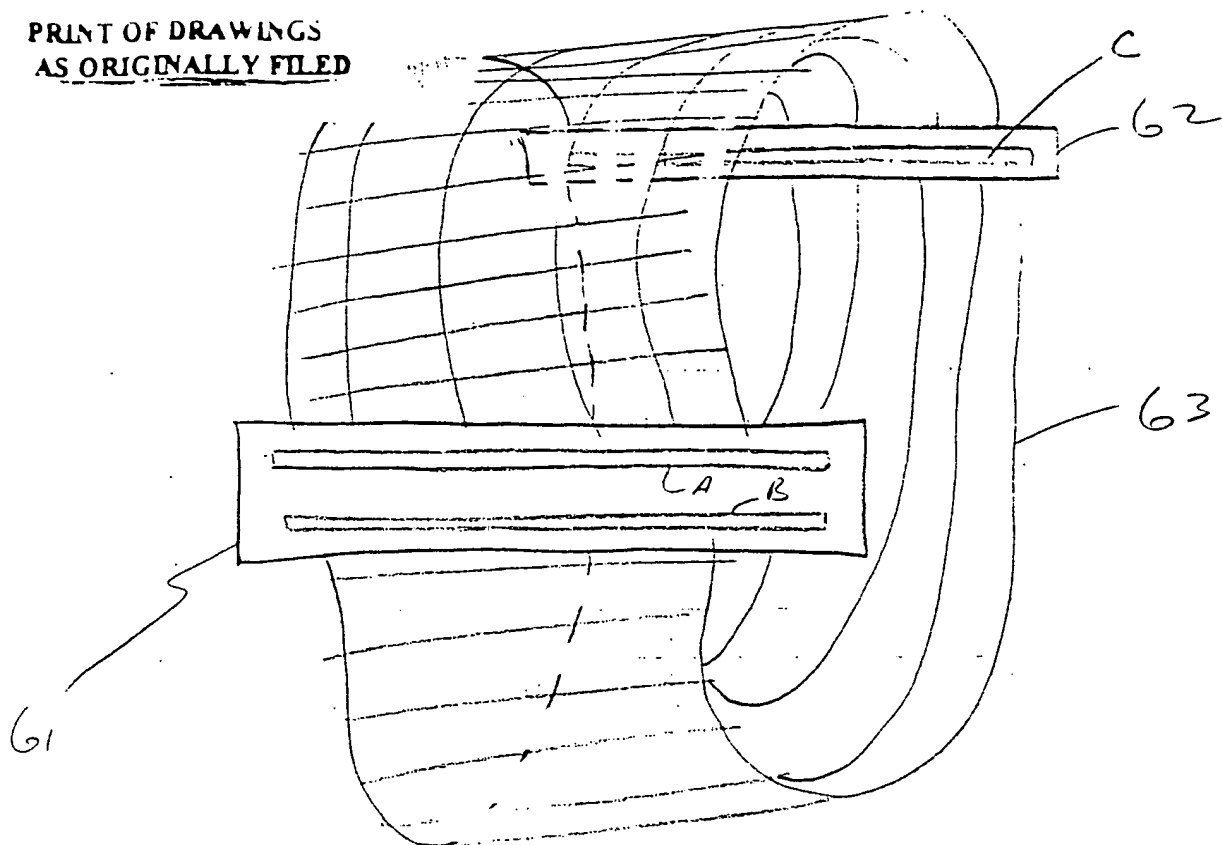


Fig. 5

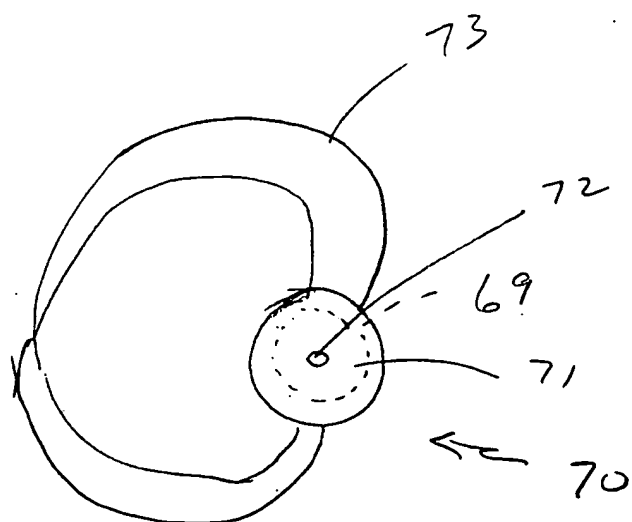


Fig. 6

00449303 112699

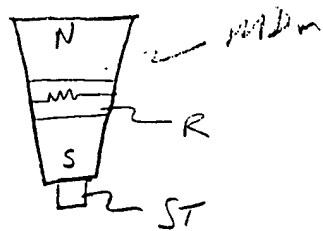
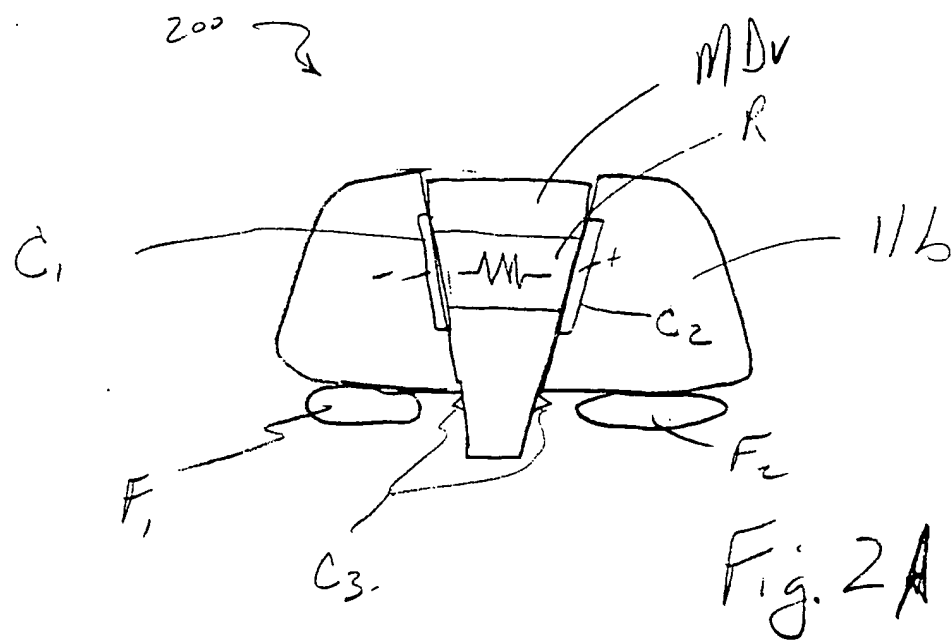


Fig 2B





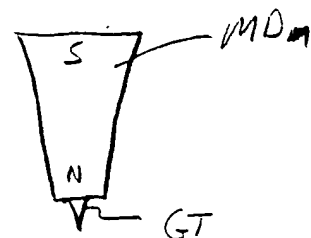


Fig 2C

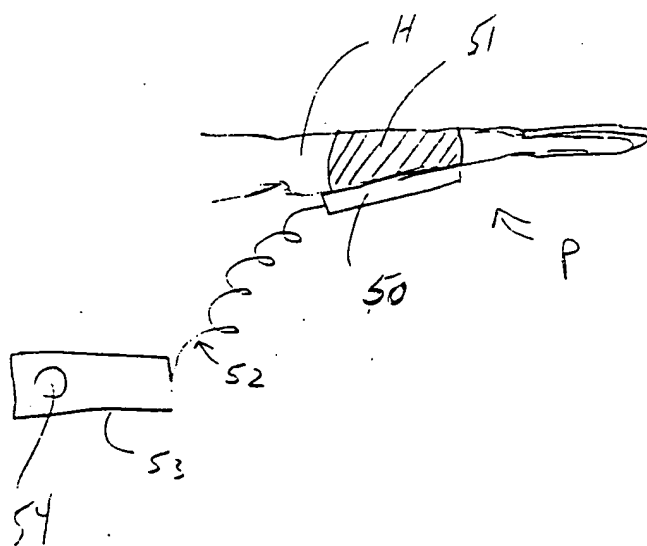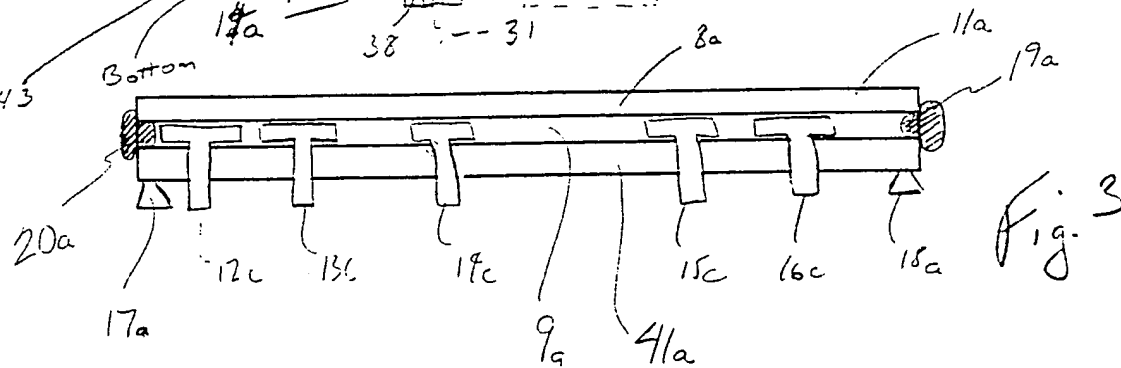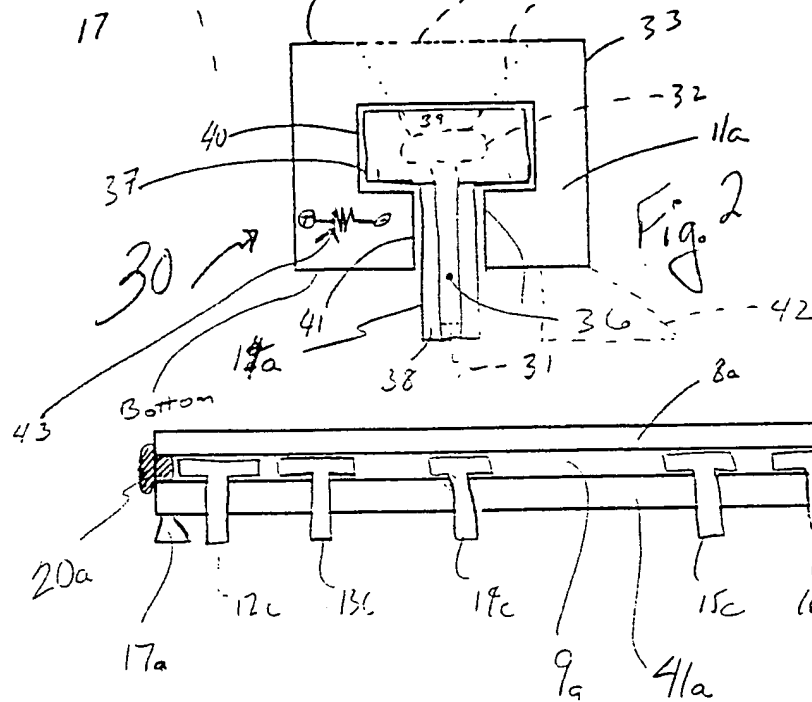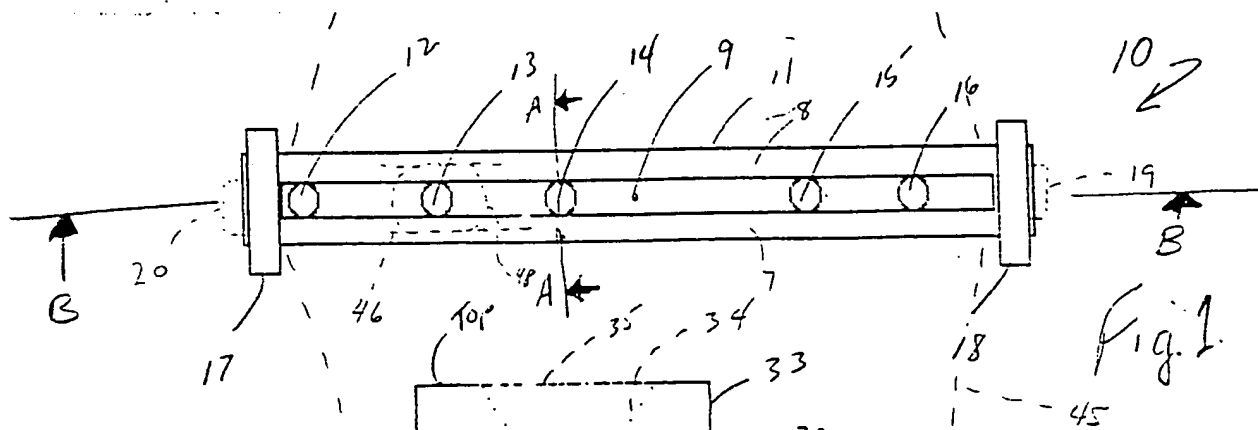

669217-12695